

# Human ACE2/ACEH Protein. Fc Tag

[www.abwizbio.com](http://www.abwizbio.com)

Support: [info@abwizbio.com](mailto:info@abwizbio.com)

Order: [sales@abwizbio.com](mailto:sales@abwizbio.com)


Catalog: #2566

Store at: 2-8°C


For Research Use Only. Not For Use In Diagnostic Procedures.

Applications	Detection	Clonality	Isotype
ELISA	Anti-SARS-CoV-2 mAb	SARS-CoV-2	Other


Format:	Fc tag
Cross Reactivity:	Predicted to work with mouse, rat and other homologues.
Formulation:	1X PBS, 0.09% NaN3
Preparation:	Protein A
Reactivity:	Human
Recommended Usage:	For SARS-CoV-2 (COVID-19) diagnostic assays.
Immunogen:	N/A
Description:	
References:	

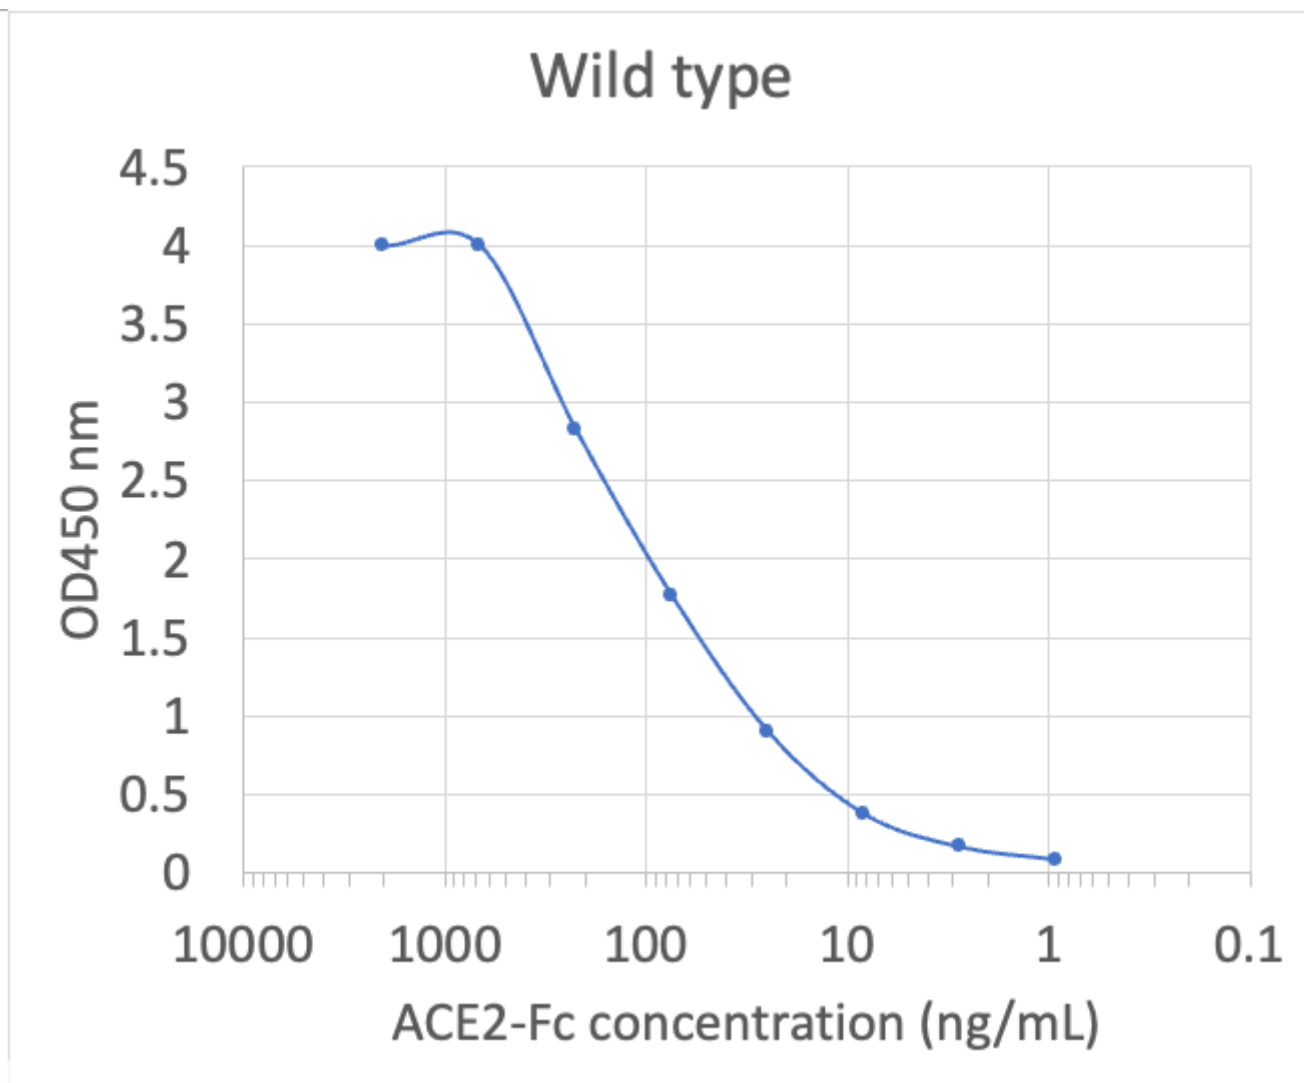

Microtiter wells were coated with 100  $\mu$ L of each spike trimer at 2  $\mu$ g/mL in PBS at 4°C overnight. The wells were washed with PBS and blocked with 200  $\mu$ L of 1% BSA/PBS. ACE2-Fc was serially diluted from 2  $\mu$ g/mL in 1% BSA/PBS. The blocker was discarded, and the wells were incubated with 100  $\mu$ L of serially diluted ACE2-Fc at 37°C for 1 hour. The wells were washed with PBS and the bound ACE2-Fc was detected with 100  $\mu$ L of Peroxidase AffiniPure Goat Anti-Human IgG, Fc $\gamma$  fragment specific (Jackson Immuno Research 109-035-098)(1:5,000 in 1% BSA/PBS) at 37°C for 1 hour. The wells were washed with PBS and the wells were developed with 100  $\mu$ L of MB/E Ultra Sensitive, Blue, Horseradish Peroxidase Substrate (EMD Millipore ES022-500ml) at RT for 5 min. The reaction was stopped with 100  $\mu$ L of 0.6N H<sub>2</sub>SO<sub>4</sub> and the signals were read at 450 nm using a plate reader (Biotek).

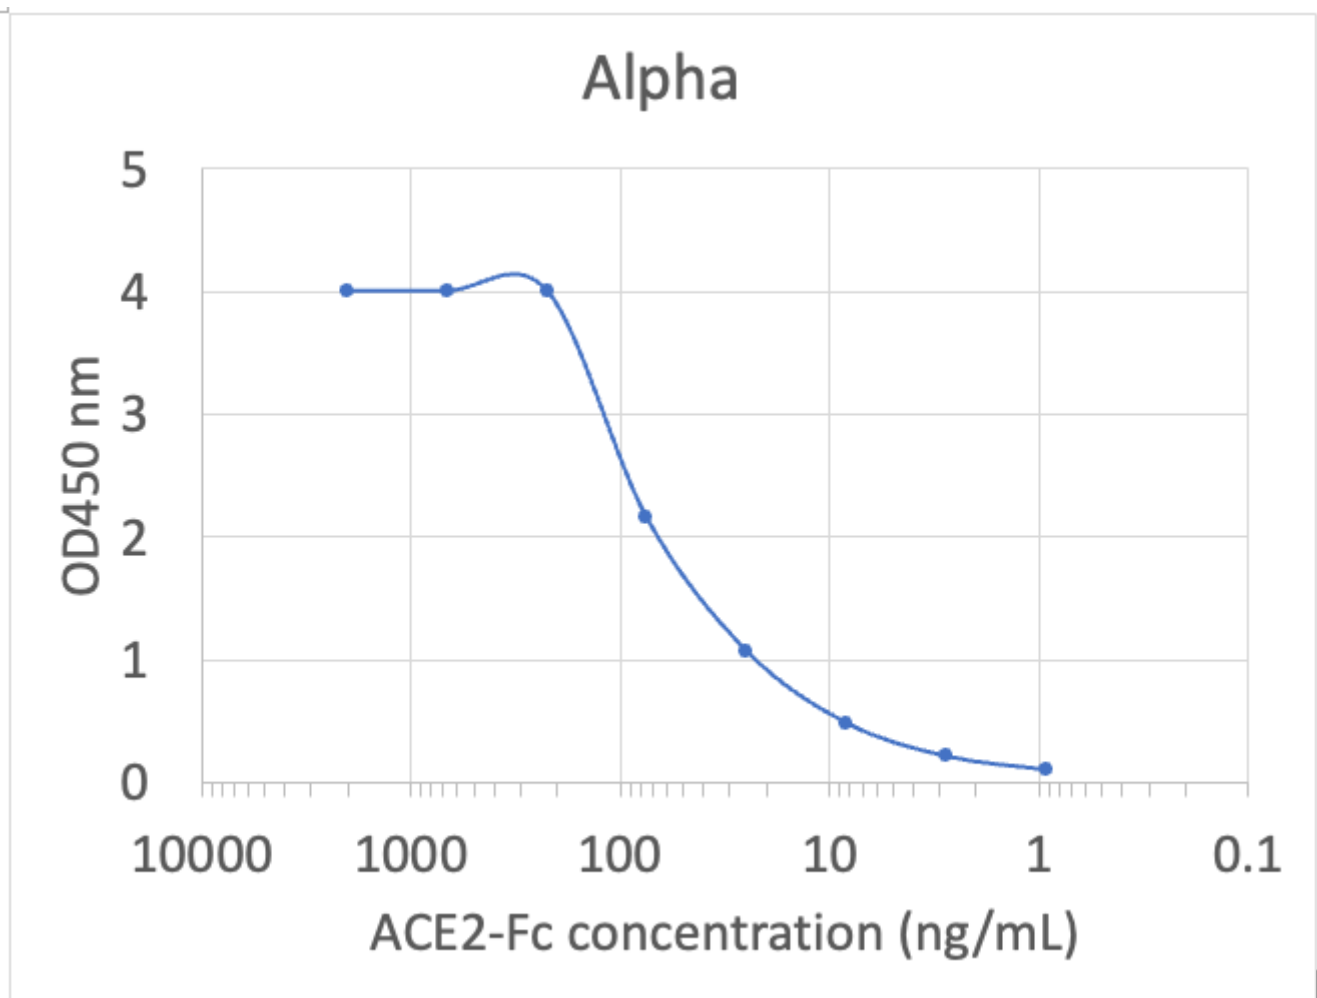


Microtiter wells were coated with 100  $\mu$ L of each spike trimer at 2  $\mu$ g/mL in PBS at 4°C overnight. The wells were washed with PBS and blocked with 200  $\mu$ L of 1% BSA/PBS. ACE2-Fc was serially diluted from 2  $\mu$ g/mL in 1% BSA/PBS. The blocker was discarded, and the wells were incubated with 100  $\mu$ L of serially diluted ACE2-Fc at 37°C for 1 hour. The wells were washed with PBS and the bound ACE2-Fc was detected with 100  $\mu$ L of Peroxidase AffiniPure Goat Anti-Human IgG, Fc $\gamma$  fragment specific (Jackson Immuno Research 109-035-098)(1:5,000 in 1% BSA/PBS) at 37°C for 1 hour. The wells were washed with PBS and the wells were developed with 100  $\mu$ L of MB/E Ultra Sensitive, Blue, Horseradish Peroxidase Substrate (EMD Millipore ES022-500ml) at RT for 5 min. The reaction was stopped with 100  $\mu$ L of 0.6N H<sub>2</sub>SO<sub>4</sub> and the signals were read at 450 nm using a plate reader (Biotek).

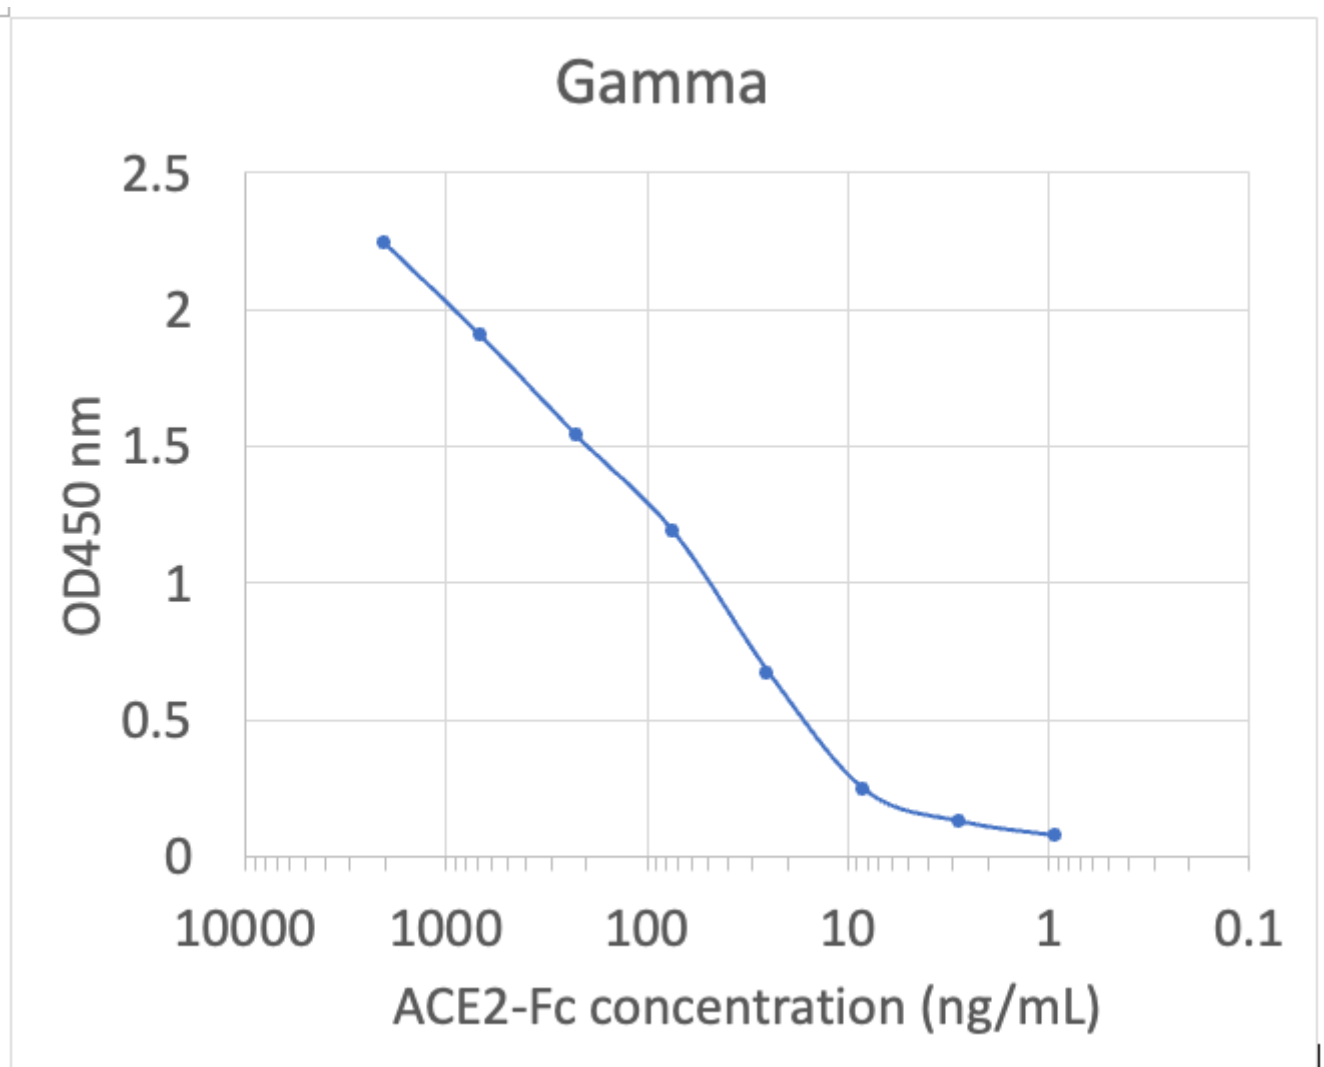


Microtiter wells were coated with 100  $\mu$ L of each spike trimer at 2  $\mu$ g/mL in PBS at 4°C overnight. The wells were washed with PBS and blocked with 200  $\mu$ L of 1% BSA/PBS. ACE2-Fc was serially diluted from 2  $\mu$ g/mL in 1% BSA/PBS. The blocker was discarded, and the wells were incubated with 100  $\mu$ L of serially diluted ACE2-Fc at 37°C for 1 hour. The wells were washed with PBS and the bound ACE2-Fc was detected with 100  $\mu$ L of Peroxidase AffiniPure Goat Anti-Human IgG, Fc $\gamma$  fragment specific (Jackson Immuno Research 109-035-098)(1:5,000 in 1% BSA/PBS) at 37°C for 1 hour. The wells were washed with PBS and the wells were developed with 100  $\mu$ L of MB/E Ultra Sensitive, Blue, Horseradish Peroxidase Substrate (EMD Millipore ES022-500ml) at RT for 5 min. The reaction was stopped with 100  $\mu$ L of 0.6N H<sub>2</sub>SO<sub>4</sub> and the signals were read at 450 nm using a plate reader (Biotek).


## Epsilon (B.1.427)

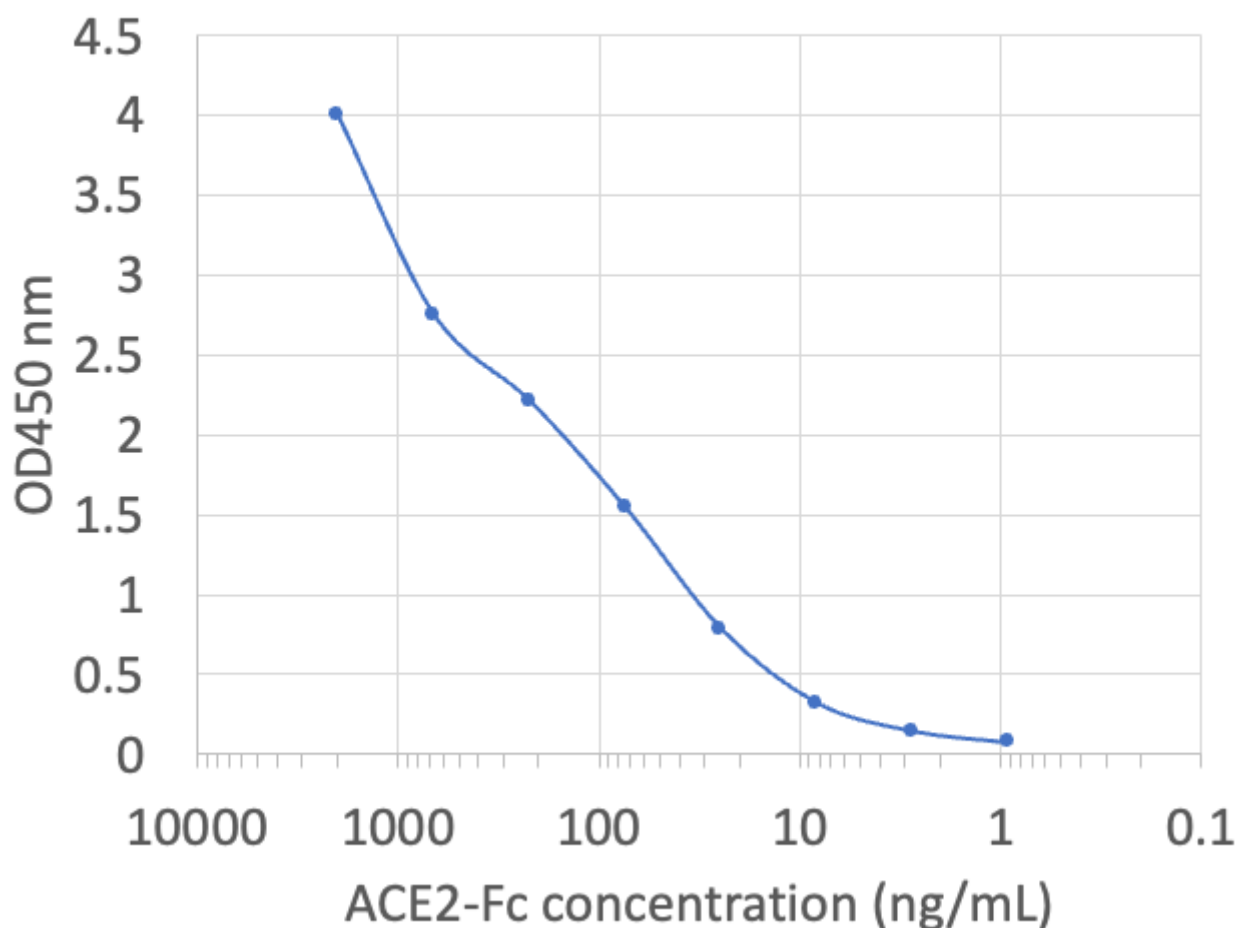


Microtiter wells were coated with 100  $\mu$ L of each spike trimer at 2  $\mu$ g/mL in PBS at 4°C overnight. The wells were washed with PBS and blocked with 200  $\mu$ L of 1% BSA/PBS. ACE2-Fc was serially diluted from 2  $\mu$ g/mL in 1% BSA/PBS. The blocker was discarded, and the wells were incubated with 100  $\mu$ L of serially diluted ACE2-Fc at 37°C for 1 hour. The wells were washed with PBS and the bound ACE2-Fc was detected with 100  $\mu$ L of Peroxidase AffiniPure Goat Anti-Human IgG, Fc $\gamma$  fragment specific (Jackson Immuno Research 109-035-098)(1:5,000 in 1% BSA/PBS) at 37°C for 1 hour. The wells were washed with PBS and the wells were developed with 100  $\mu$ L of MB/E Ultra Sensitive, Blue, Horseradish Peroxidase Substrate (EMD Millipore ES022-500ml) at RT for 5 min. The reaction was stopped with 100  $\mu$ L of 0.6N H<sub>2</sub>SO<sub>4</sub> and the signals were read at 450 nm using a plate reader (Biotek).

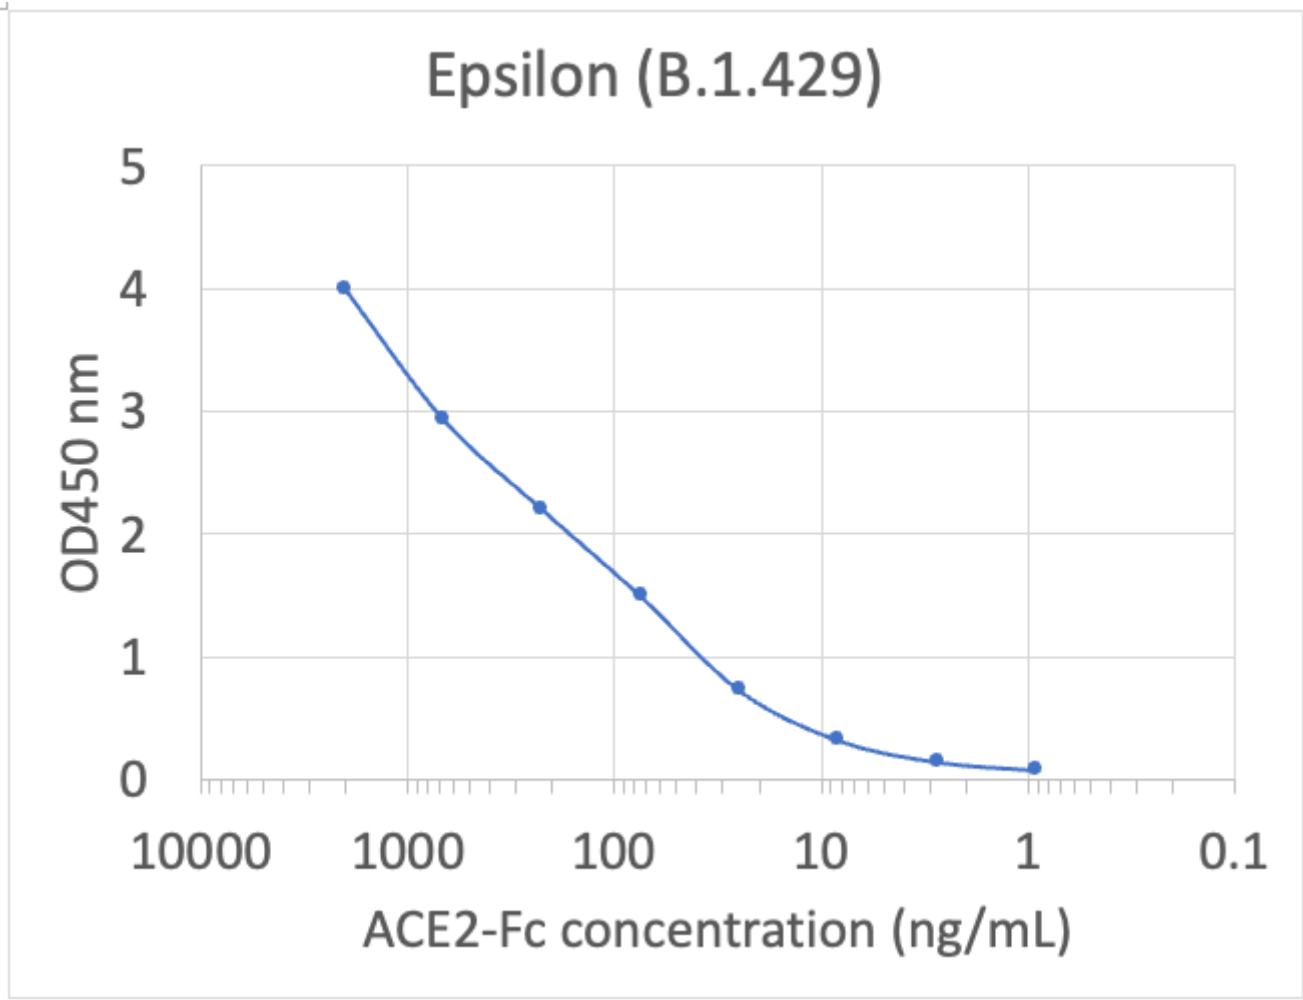

Microtiter wells were coated with 100  $\mu$ L of each spike trimer at 2  $\mu$ g/mL in PBS at 4°C overnight. The wells were washed with PBS and blocked with 200  $\mu$ L of 1% BSA/PBS. ACE2-Fc was serially diluted from 2  $\mu$ g/mL in 1% BSA/PBS. The blocker was discarded, and the wells were incubated with 100  $\mu$ L of serially diluted ACE2-Fc at 37°C for 1 hour. The wells were washed with PBS and the bound ACE2-Fc was detected with 100  $\mu$ L of Peroxidase AffiniPure Goat Anti-Human IgG, Fc $\gamma$  fragment specific (Jackson Immuno Research 109-035-098)(1:5,000 in 1% BSA/PBS) at 37°C for 1 hour. The wells were washed with PBS and the wells were developed with 100  $\mu$ L of MB/E Ultra Sensitive, Blue, Horseradish Peroxidase Substrate (EMD Millipore ES022-500ml) at RT for 5 min. The reaction was stopped with 100  $\mu$ L of 0.6N H<sub>2</sub>SO<sub>4</sub> and the signals were read at 450 nm using a plate reader (Biotek).

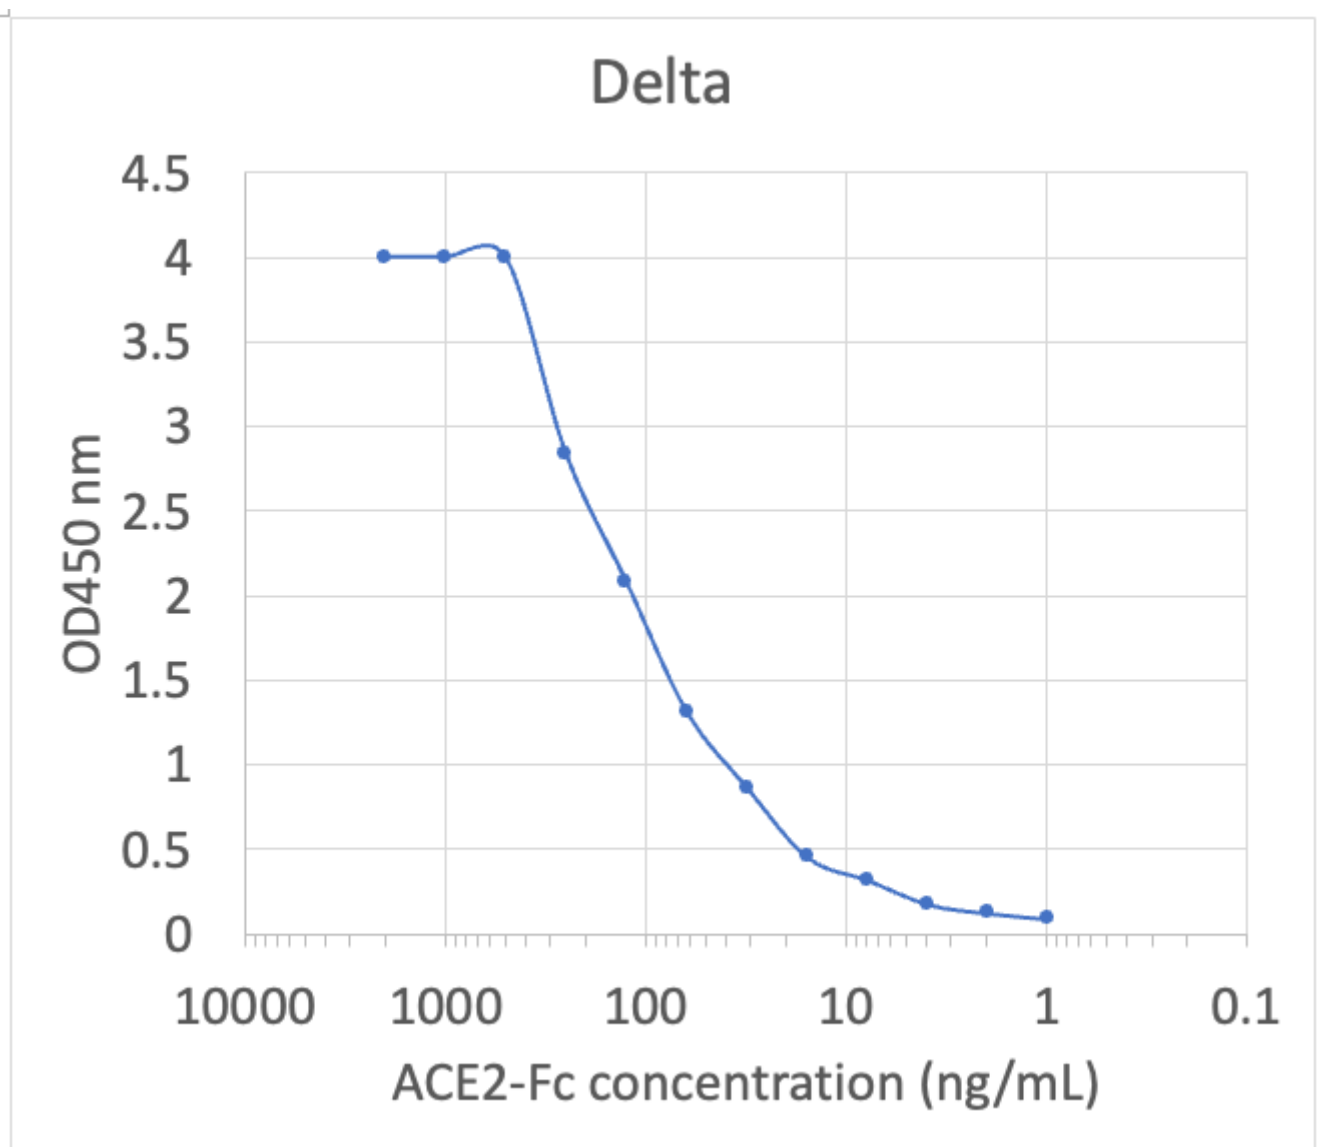

Microtiter wells were coated with 100  $\mu$ L of each spike trimer at 2  $\mu$ g/mL in PBS at 4°C overnight. The wells were washed with PBS and blocked with 200  $\mu$ L of 1% BSA/PBS. ACE2-Fc was serially diluted from 2  $\mu$ g/mL in 1% BSA/PBS. The blocker was discarded, and the wells were incubated with 100  $\mu$ L of serially diluted ACE2-Fc at 37°C for 1 hour. The wells were washed with PBS and the bound ACE2-Fc was detected with 100  $\mu$ L of Peroxidase AffiniPure Goat Anti-Human IgG, Fc $\gamma$  fragment specific (Jackson Immuno Research 109-035-098)(1:5,000 in 1% BSA/PBS) at 37°C for 1 hour. The wells were washed with PBS and the wells were developed with 100  $\mu$ L of MB/E Ultra Sensitive, Blue, Horseradish Peroxidase Substrate (EMD Millipore ES022-500ml) at RT for 5 min. The reaction was stopped with 100  $\mu$ L of 0.6N H<sub>2</sub>SO<sub>4</sub> and the signals were read at 450 nm using a plate reader (Biotek).

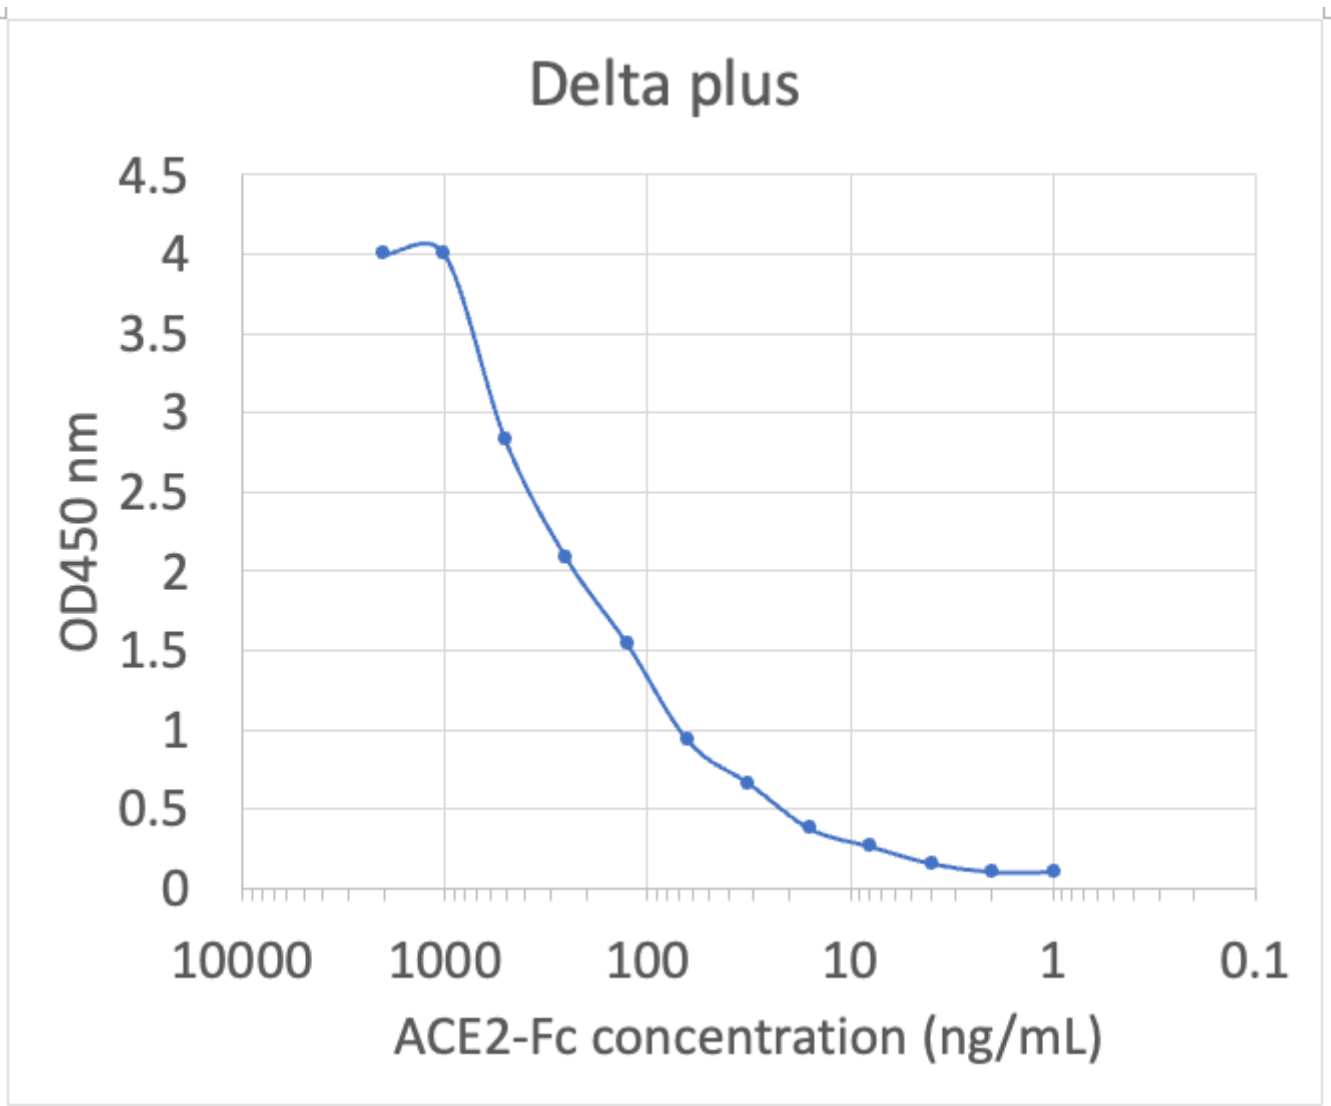

Microtiter wells were coated with 100  $\mu$ L of each spike trimer at 2  $\mu$ g/mL in PBS at 4°C overnight. The wells were washed with PBS and blocked with 200  $\mu$ L of 1% BSA/PBS. ACE2-Fc was serially diluted from 2  $\mu$ g/mL in 1% BSA/PBS. The blocker was discarded, and the wells were incubated with 100  $\mu$ L of serially diluted ACE2-Fc at 37°C for 1 hour. The wells were washed with PBS and the bound ACE2-Fc was detected with 100  $\mu$ L of Peroxidase AffiniPure Goat Anti-Human IgG, Fc $\gamma$  fragment specific (Jackson Immuno Research 109-035-098)(1:5,000 in 1% BSA/PBS) at 37°C for 1 hour. The wells were washed with PBS and the wells were developed with 100  $\mu$ L of MB/E Ultra Sensitive, Blue, Horseradish Peroxidase Substrate (EMD Millipore ES022-500ml) at RT for 5 min. The reaction was stopped with 100  $\mu$ L of 0.6N H<sub>2</sub>SO<sub>4</sub> and the signals were read at 450 nm using a plate reader (Biotek).